


赫兹电力
HERTZ POWER

HZJYY-JT

赫兹电力
HERTZ POWER



.....	2
.....	2
.....	3
.....	3
.....	4
.....	5
.....	9

赫兹电力
HERTZ POWER



02



1

2

PID


—D

赫兹电力
HERTZ POWER





赫兹电力
HERTZ POWER



±

±

±

±

m "

7



赫兹电力
HERTZ POWER

,0'000 ' w .. U

0 ‡ KOT


000

027-83267669


www.whhezi.com

whhezi@163.com


1

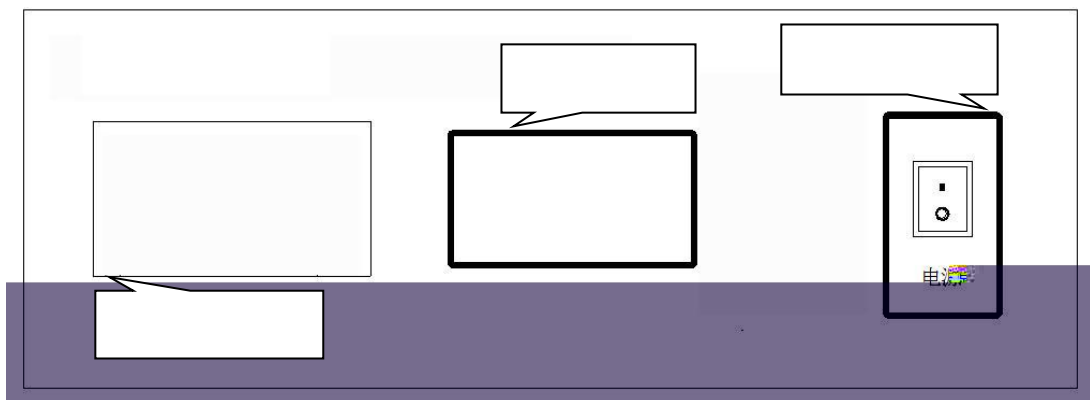

1

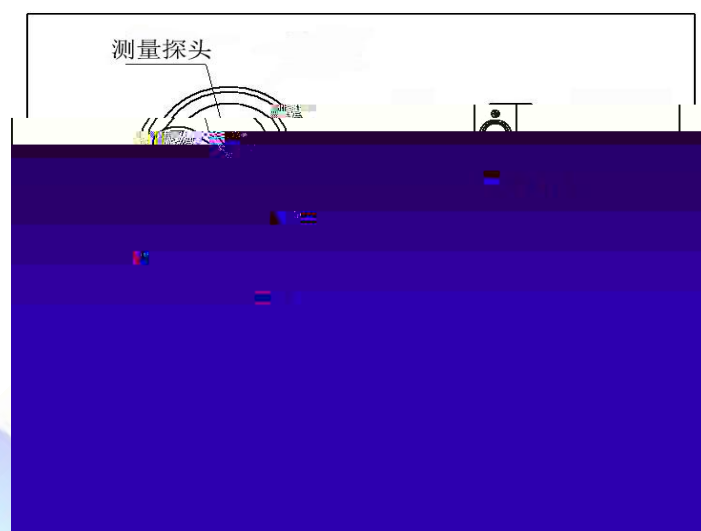

2

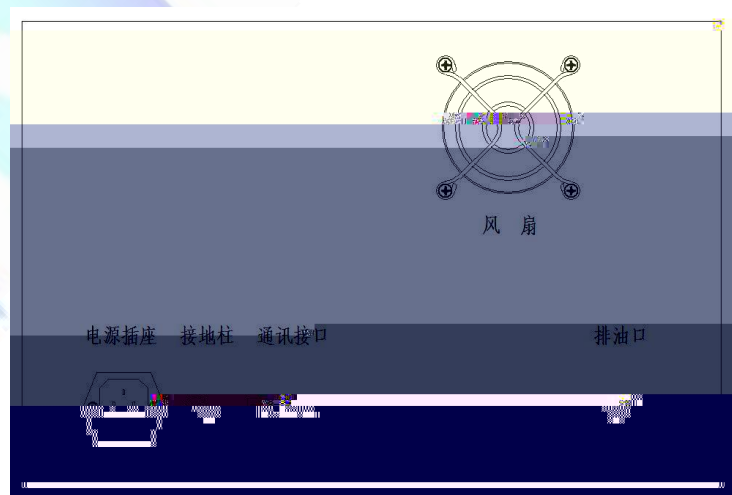

3

2

AC220V




1

2

2

4

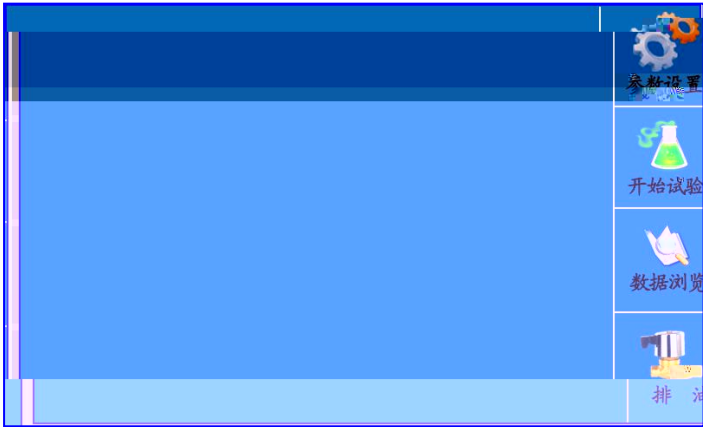

4

3

5



5

4





/

/

/

介质损耗因数测量

介质损耗 0.000 %

当前温度 33.3 C

设置温度 20.0 C

介质损耗因数 0.000 %

9-1

直流电阻率测量

设置温度 90 °C

当前温度 33.3 °C

设置电压 2000 V

当前电压 333 V


正在测试

停止

返回

9-2


10

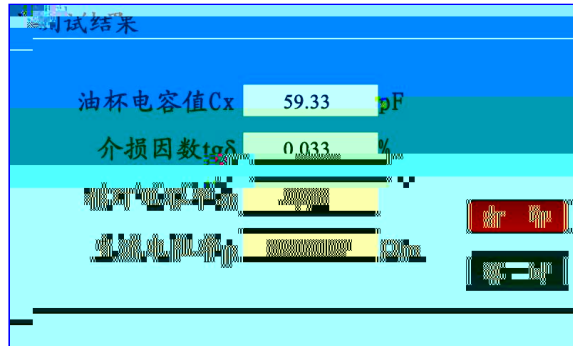

10

6

11

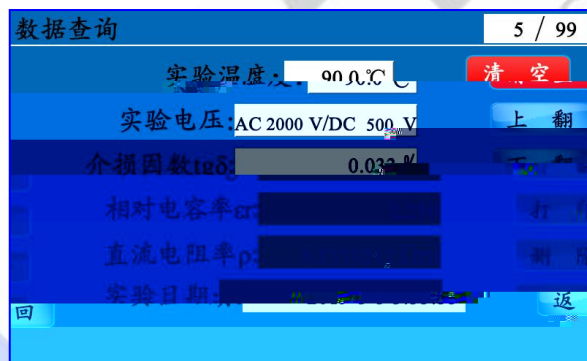


11

100

: 6+

1

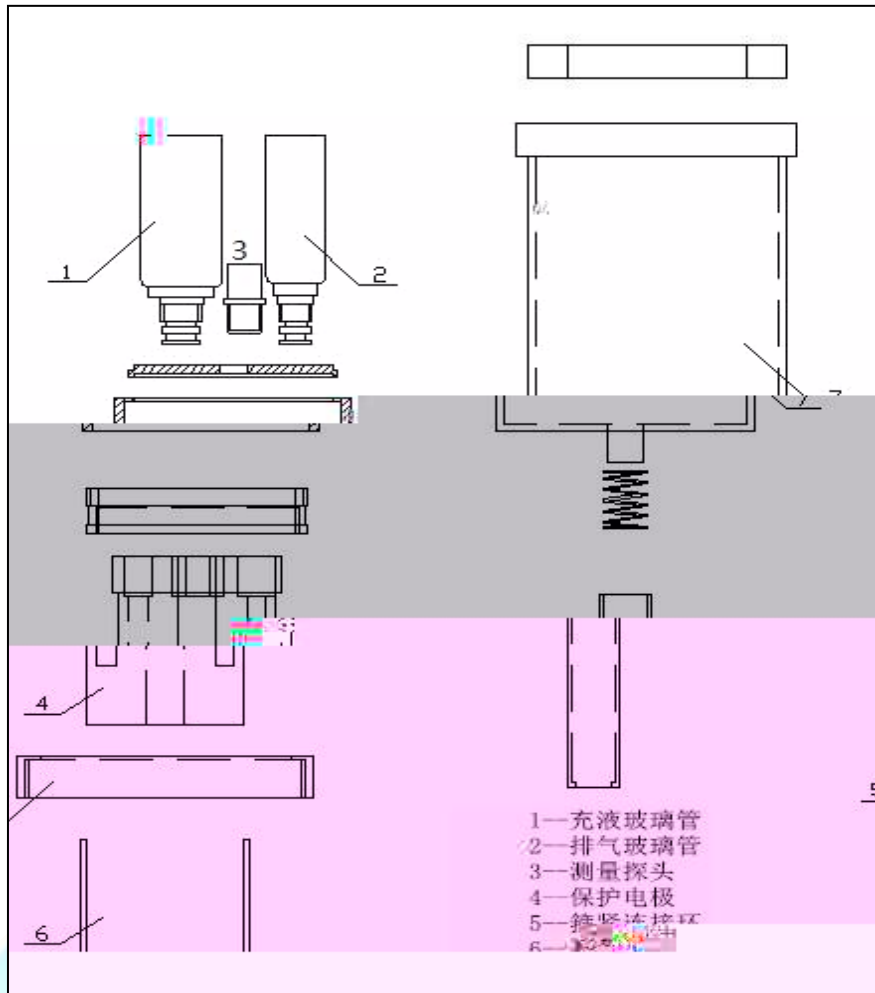

13

2

±

$\delta \times$

$\times$

225

027-83267669



5

20

威兹电力
WHEZI POWER

“

”

“

”

1

2

1.

2.



1

2

3

2

24

027-83267669

24

48

4